

SEILERSCOPE

COMPOUND MICROSCOPE USER'S MANUAL



This document is property of Seiler Instrument & Mfg. Co., Inc. No part of this manual should be reproduced or transmitted without the expressed written consent being obtained. All the figures appearing in this manual are for illustration purposes only and may vary according to the version of the device purchased. The information contained in this manual is subject to change without notice. Please contact Seiler whenever additional information is needed. This device is restricted to the sale and the use by authorized and trained personnel.

TABLE OF CONTENTS

SPECIFICATIONS.....4

COMPONENTS.....5

OPTICAL SYSTEM9

OBSERVING OPERATION.....10

EXCHANGING THE LAMP AND FUSE.....13

CIRCUIT DIAGRAM.....14

TIPS & TECHNIQUES15

WARRANTIES 16-17

We are here to serve you!

If you have any questions regarding Seiler’s products or services,
please feel free to contact us.

Toll-Free: 800.489.2282
Local: 314.968.2282
Fax: 314.968.3601
www.seilerinst.com



Register your product warranty online:
<http://www.seilermicro.com/warranty-registration/>

INTRODUCTION

To Our Valued Professionals,

On behalf of the Seiler Medical Division, I would like to thank you for your recent purchase. We stand by our products and are thrilled that when choosing one of the most important aspects of your practice, you chose us.

We are proud to say that, as a company, we have over 70 years' experience in the optical field. We have the expertise to provide you with modern, reliable devices that incorporate some of the most advanced optical design tools on the market. This product's intent is to amplify an image while providing the user with an exceptional level of comfort, improved visual acuity, and provide flawless maneuverability for any office or hospital.

All of our products are manufactured according to strict medical and ISO standards. We also ensure all optical components have undergone an anti-reflective, multi-layer treatment; guaranteeing the efficiency of the system and enhancing the longevity of all of our products. Along with strict manufacturing standards and rigorous testing, we also stand behind all of our products by offering a lifetime warranty on all optics and mechanics for microscopes purchased in the United States, as well as a 3-year warranty on all international purchases.

Every Seiler Medical Division team member is here to provide you with outstanding service, quality, and knowledge. Our number one priority is, and always will be, providing 100% customer satisfaction to every one of our customers. If you need any further information about the equipment or just have a question, please contact us using the information below.

Thank you again for your purchase and we look forward to serving all of your optical needs for years to come.

Sincerely,

Dane Carlson
Medical Division Manager

Seiler Medical Division

Toll Free: (800) 489-2282

Local: (314) 968-2282

Email: micro@seilerinst.com

Web: www.seilerinst.com

THE DIVISIONS OF SEILER INSTRUMENT




Manufacturing



Geospatial



Medical



Planetarium



Design Solutions

The SeilerScope Biological Microscope is equipped with achromatic objectives and wide field eyepieces with binocular head, so the observer can get the clear image in the wide field.

SPECIFICATIONS

1. Eyepieces

Type	Magnification	Focus (mm)	Field (mm)	Remark
Plan eyepiece	10x	25	18	

2. Objectives:

Type	Magnification	N.A.	W. D. (mm)
Achromatic	4x	0.1	37.4
Achromatic	10x	0.25	6.6
Achromatic	40x	0.65	0.57
Achromatic	100x	1.25 oil	0.19

3. Total Magnification:

<div> <div>Objective</div> <div>Total Magnification</div> <div>Eyepiece</div> </div>			
	4x	10x	40x
10x	40x	100x	400x

- Condenser numerical aperture: 1.25
- Stage cross travel range: longitudinal 34mm, traverse 75mm
- Fine focusing knob: minimum division 0.002 mm.
- Interpupillary distances adjustment range: from 55 mm to 75 mm.
- Light sources: using a 6V20W Halogen lamp brightness adjustable.
- Power supply: Can be operated on AC 220V 50HZ or AC 110V 60HZ

COMPONENTS

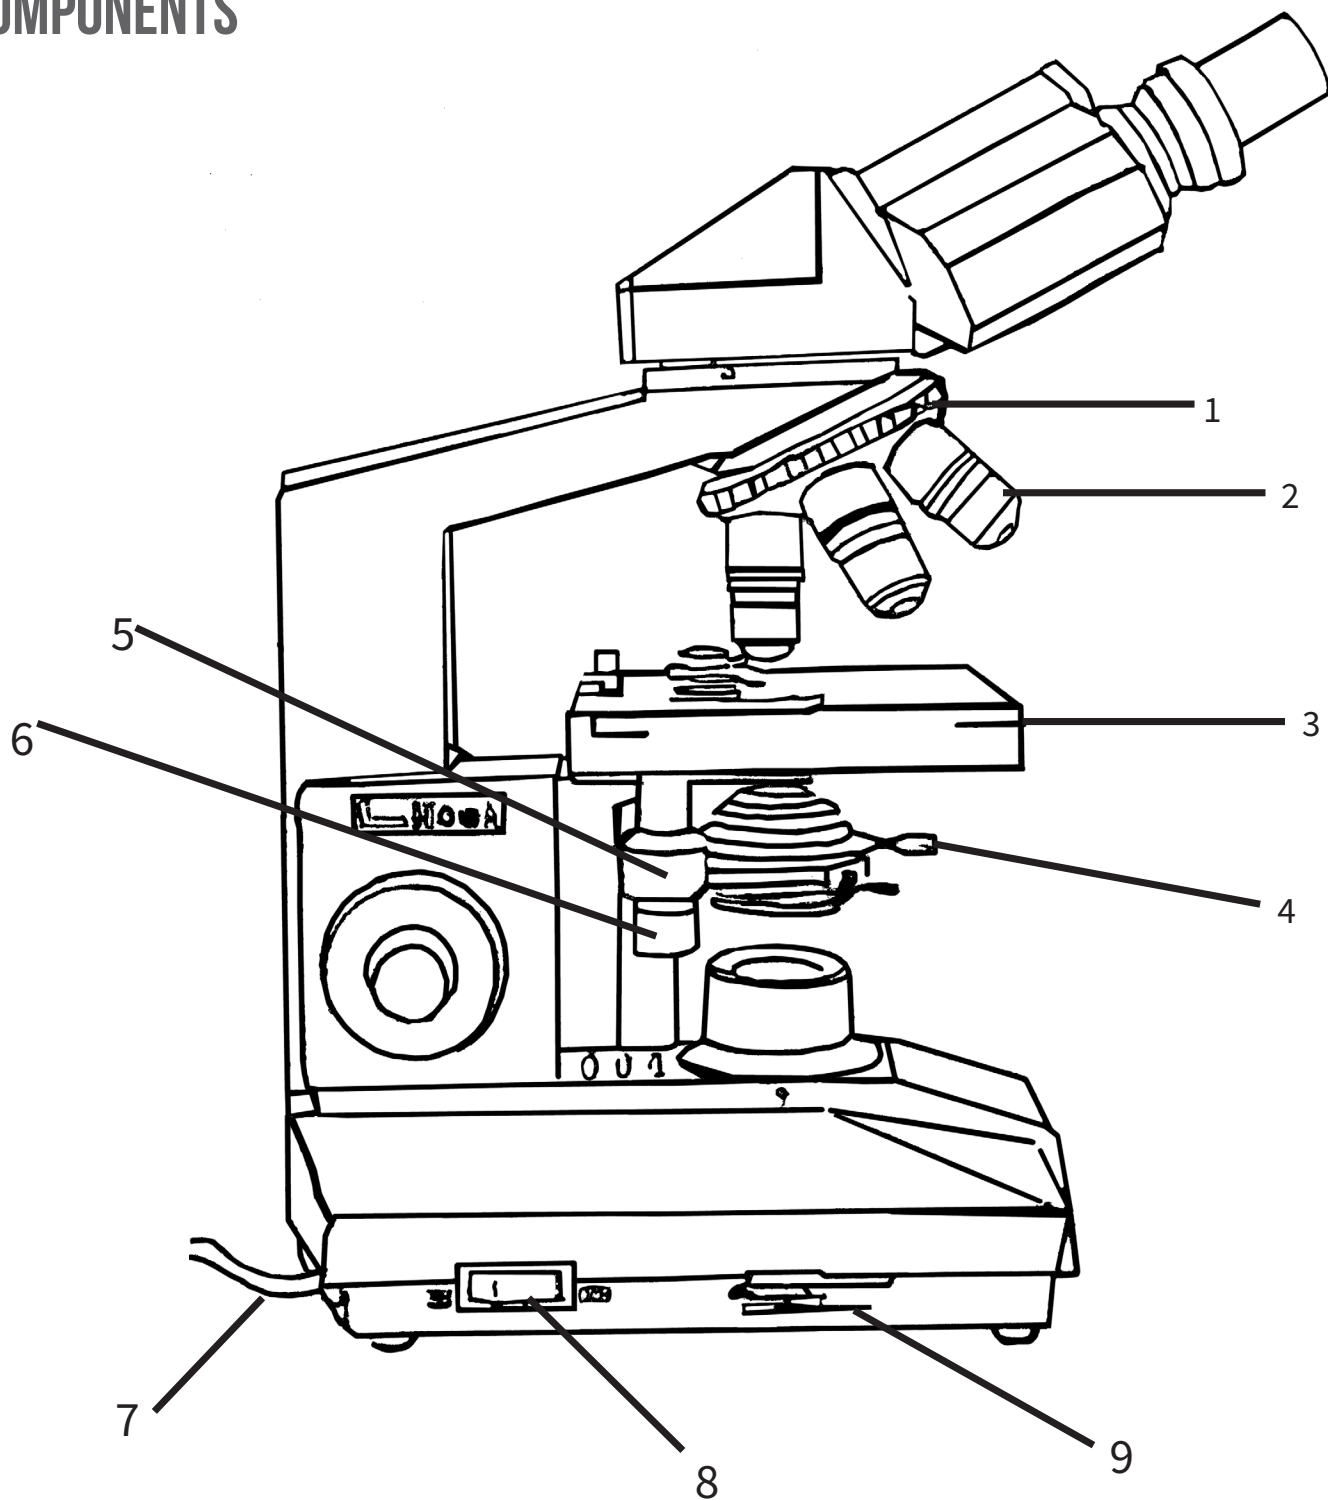


FIG. 1

1. Revolving nose-piece
2. Objectives
3. Mechanical stage
4. Condenser clipping screw
5. Shifting longitudinal controller
6. Traverse shifting controller
7. Power supply cable
8. Light source on/off
9. Brightness adjustment control lever

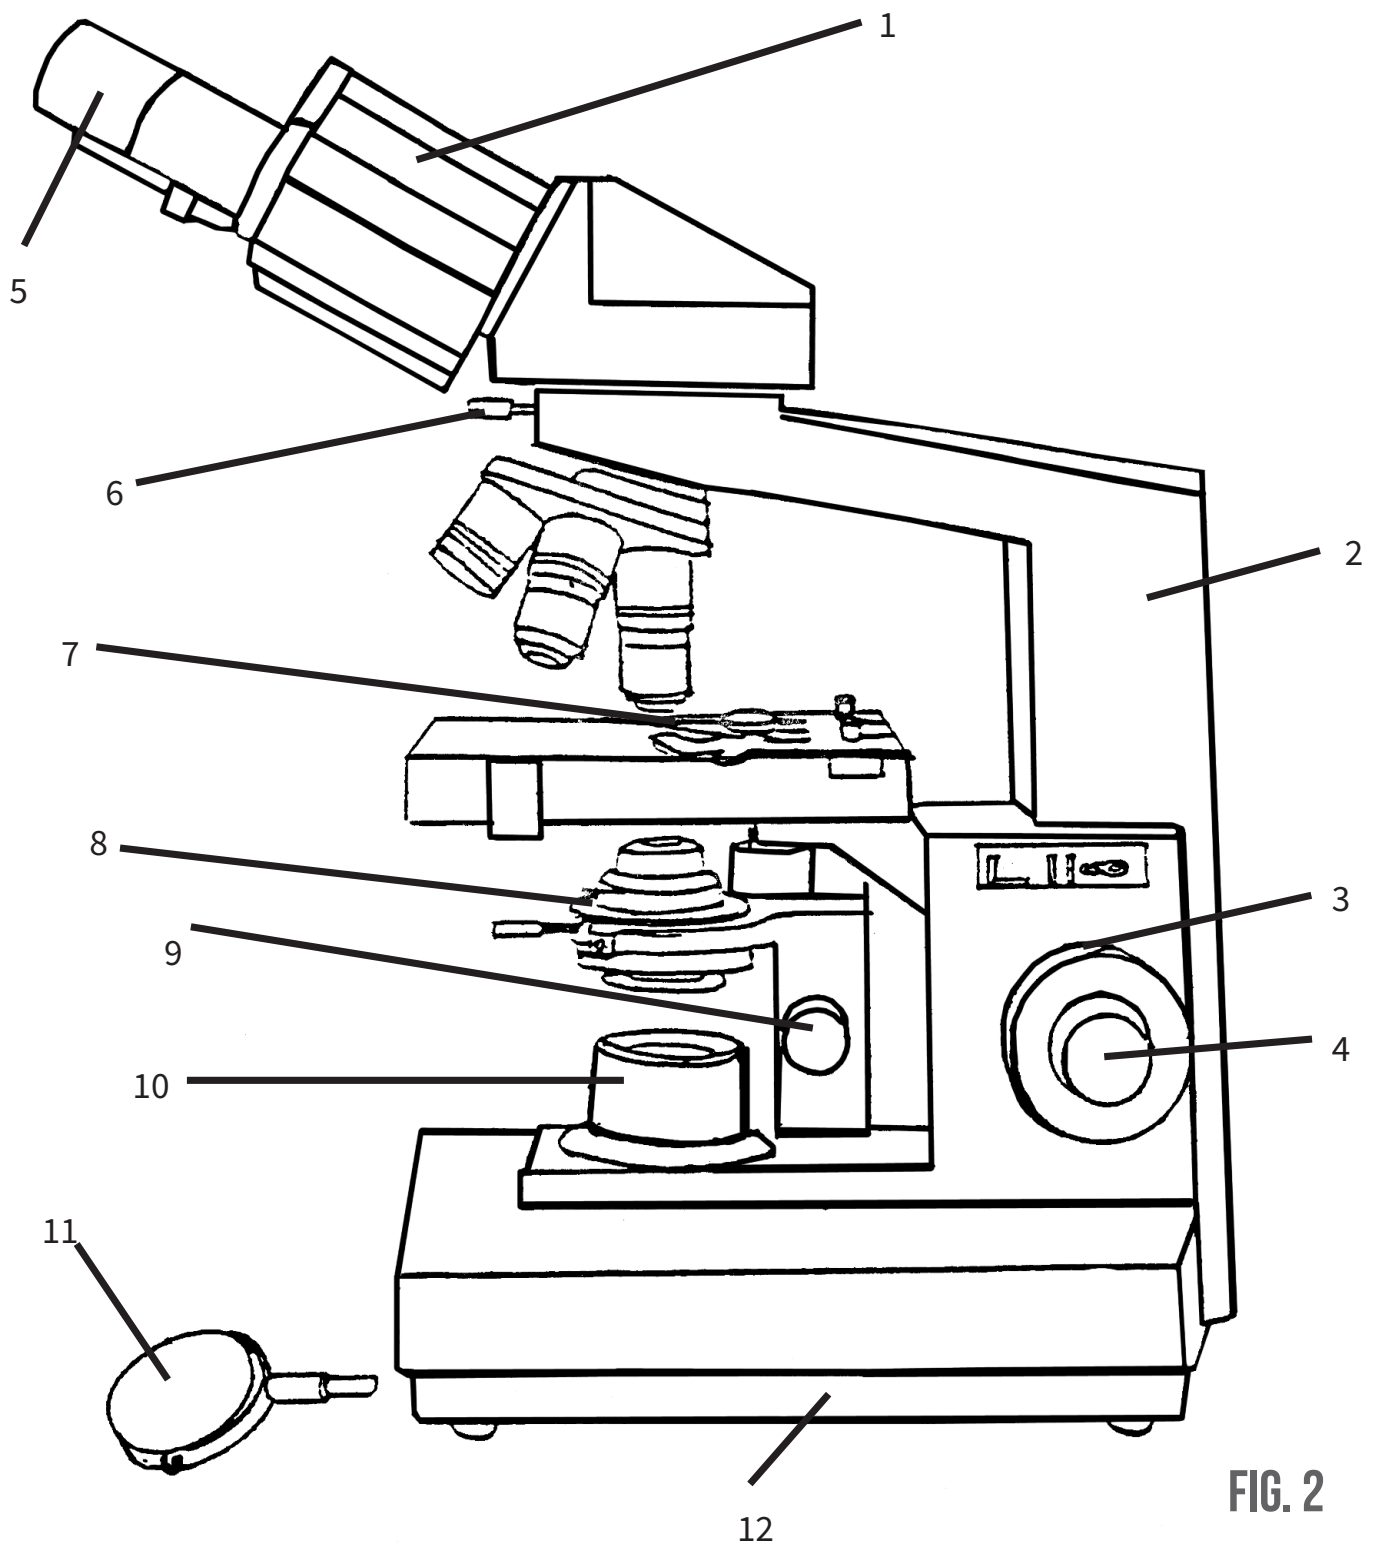


FIG. 2

- 1. Binocular
- 2. Body
- 3. Coarse focusing knob
- 4. Fine focusing knob
- 5. Eyepiece
- 6. Binocular clipping screw

- 7. Specimen cup
- 8. Condenser
- 9. Condenser up/down knob
- 10. Collector
- 11. Reflector
- 12. Base

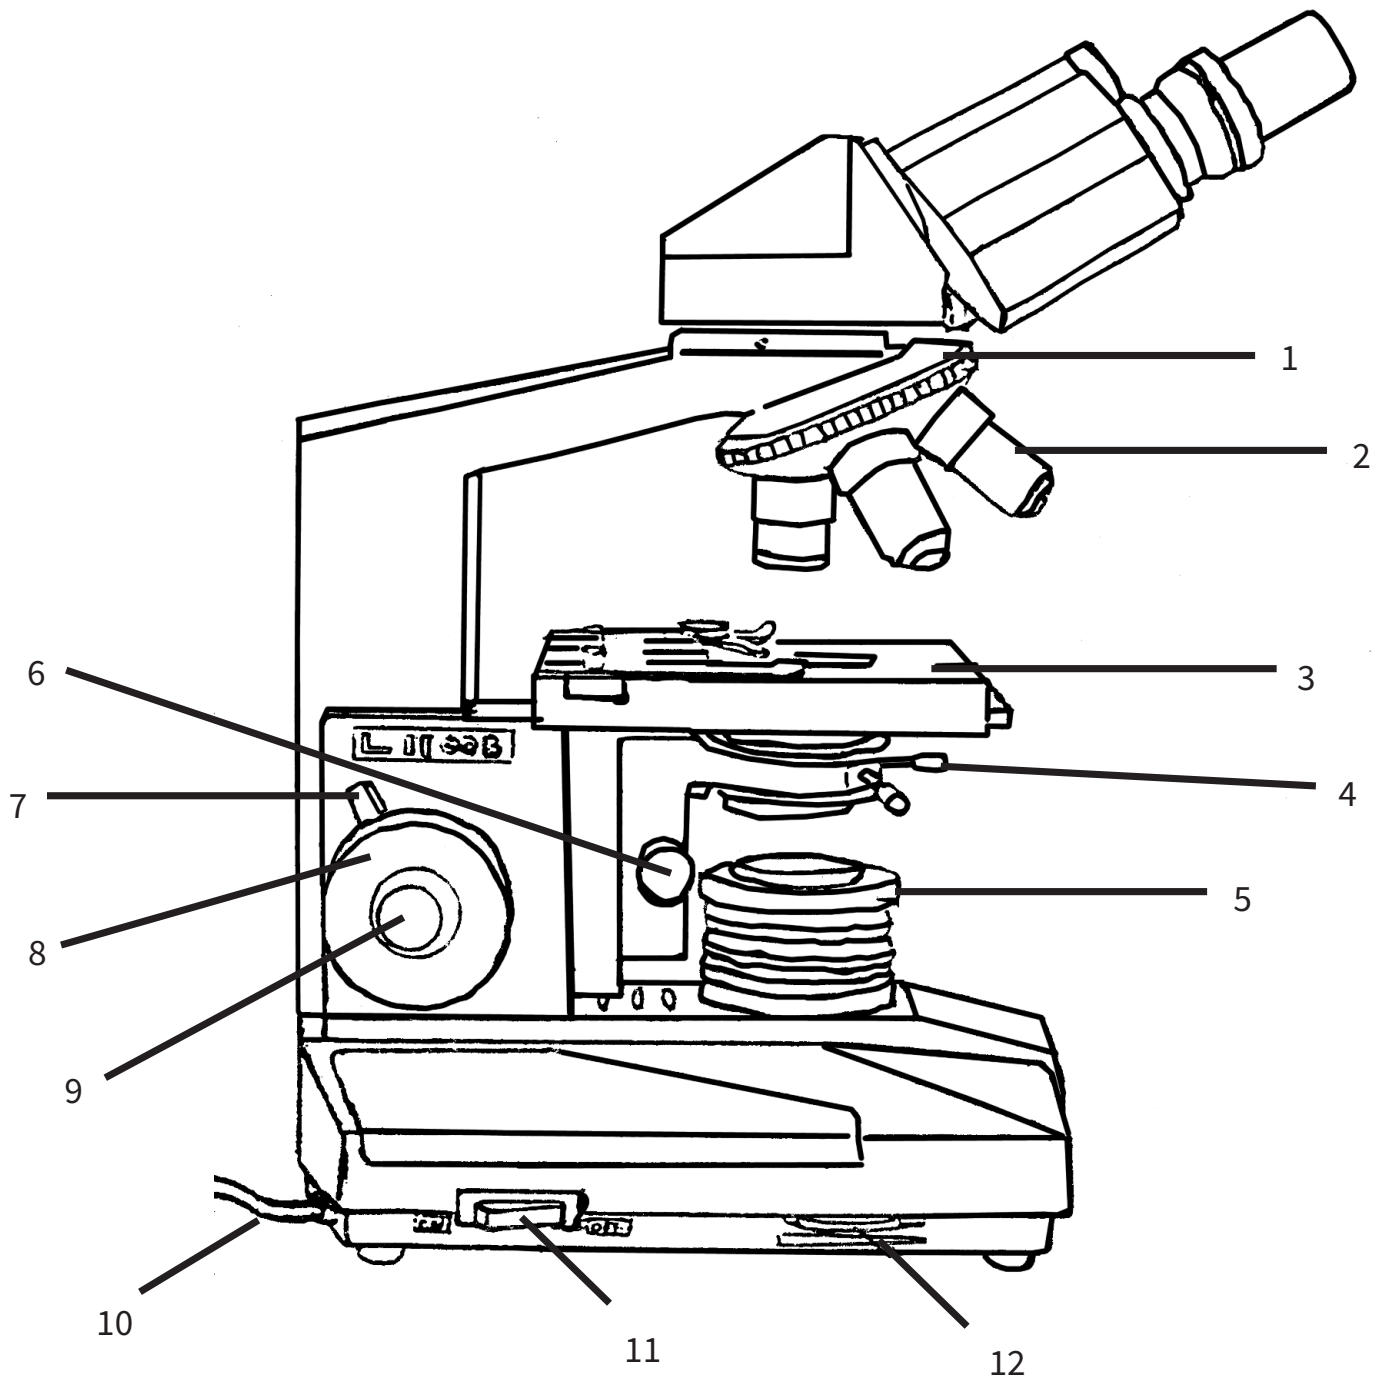


FIG. 3

1. Revolving nosepiece
2. Objectives
3. Mechanical stage
4. Condenser clipping screw
5. Field diaphragm (select)
6. Condenser up/down knob

7. Focusing limit knob
8. Coarse focusing knob
9. Fine focusing
10. Power supply cable
11. Light sources on/off
12. Brightness adjustment control lever

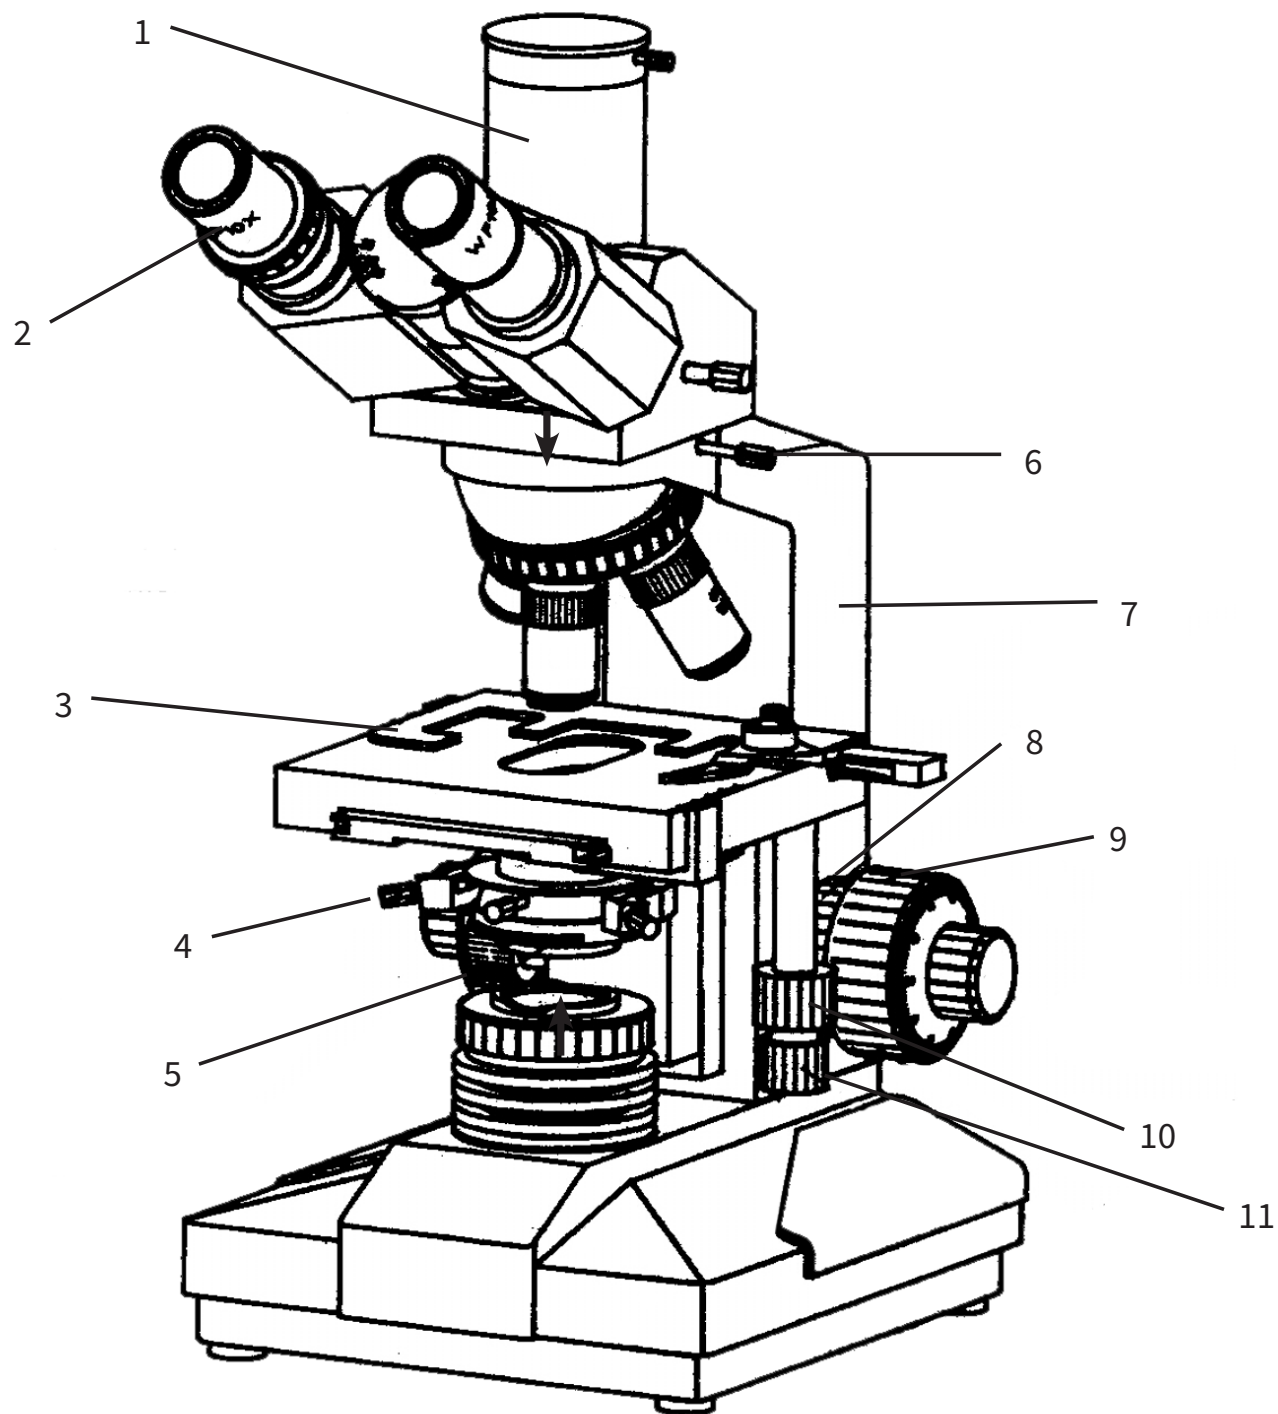


FIG. 4

- 1. Trinocular
- 2. Eyepiece
- 3. Specimen holder
- 4. Condenser adjusting screw
- 5. Condenser with aperture diaphragm
- 6. Tube holding screw

- 7. Main body
- 8. Adjustable tension knob
- 9. Coarse focusing knob
- 10. Lengthwise knob
- 11. Cross knob

OPTICAL SYSTEM

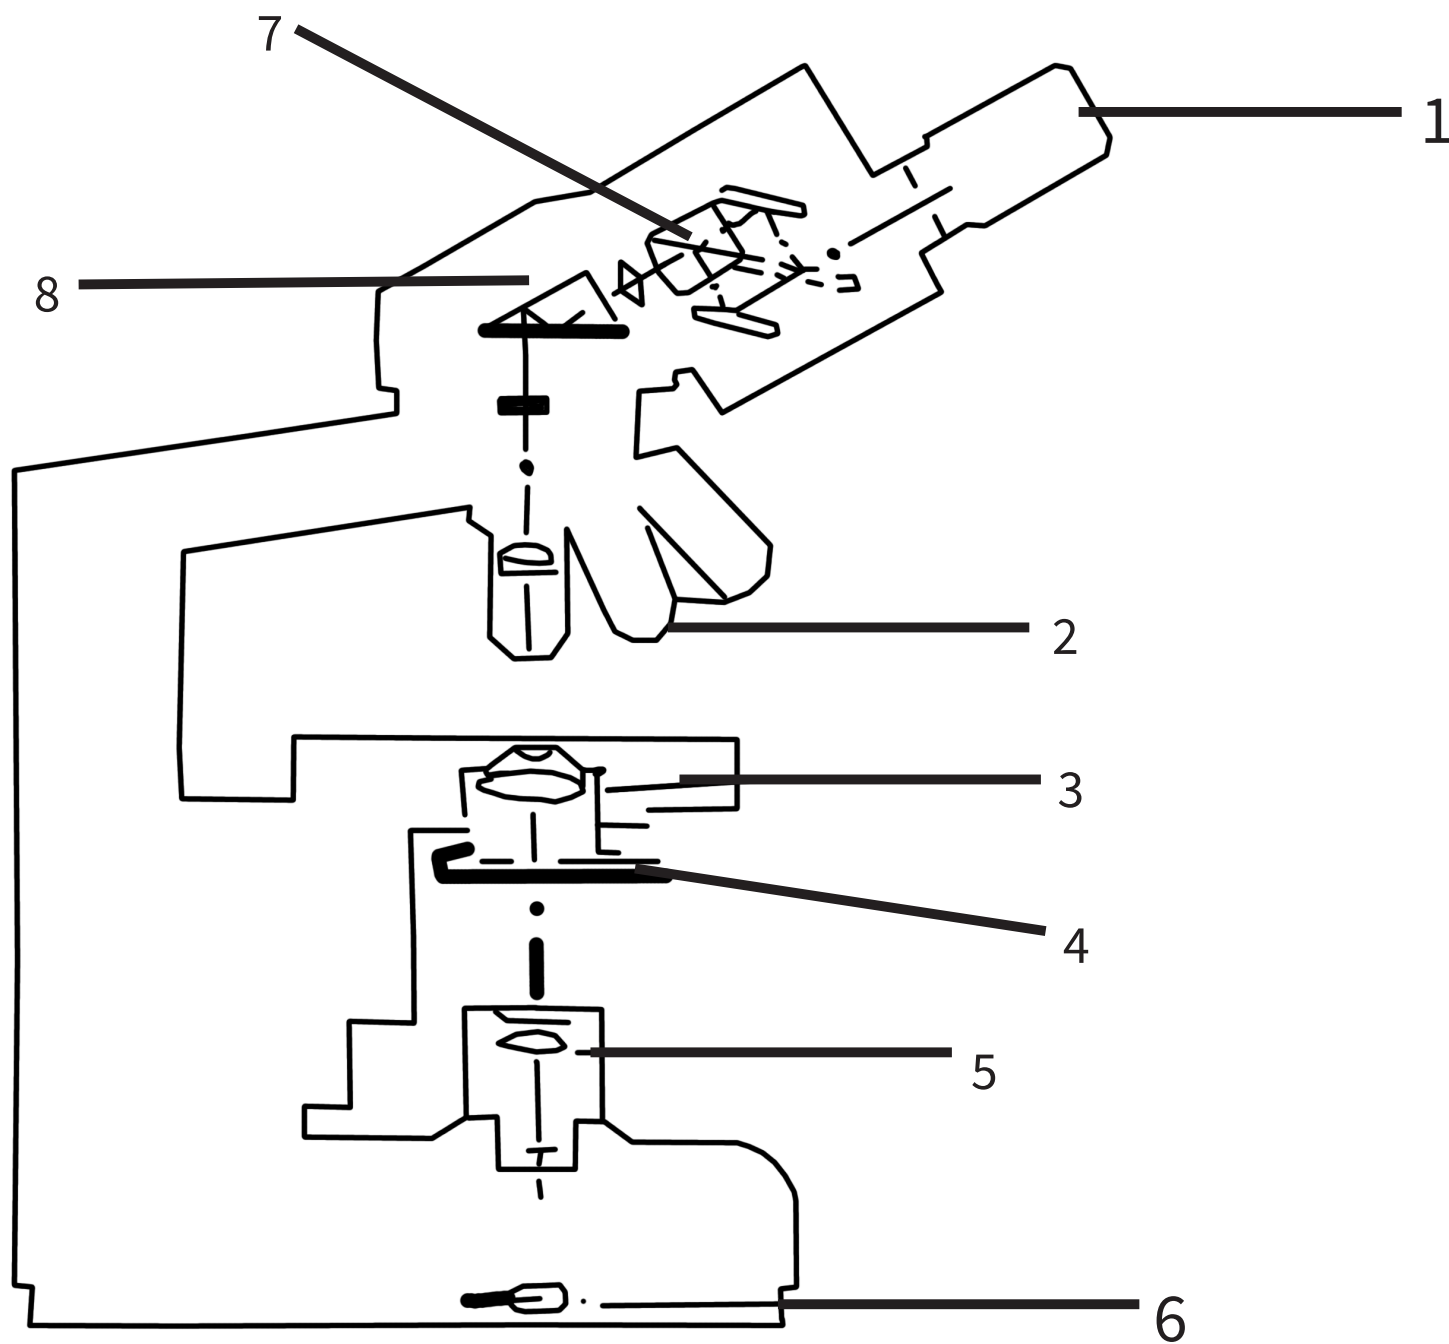


FIG. 5

- | | |
|------------------------|-----------------------|
| 1. Eyepiece | 2. Objective |
| 3. Condenser | 4. Aperture diaphragm |
| 5. Collector lens | 6. Halogen lamp |
| 7. Prism-mirror system | |

OBSERVING OPERATION

1. General operation

- (1) Turn on the power by pressing the ON/OFF switch.
- (2) Set the 10x objective into operation position by turning the nose-piece. Then focus the specimen which is on the stage.
- (3) Adjust the interdistances of binocular to fit the eyes of observer.
- (4) For desirable illumination, up or down the condenser. Vary the illumination controller and adjust aperture of the iris.
- (5) While interchange other objective, turn the nosepiece and refocus slightly with the fine focusing knob. When using the 100x immersion objective, be sure to put a drop of cedar wood oil between the objective and the specimen.

2. Setting components

- (1) Adjust the binocular for fitting the pupil distances. Focus the specimen and combine the left and right view fields into one by adjusting the interdistances of the binocular. (shown in Fig. 6)
- (2) Fit the binocular's to observer's sight. Observe with right eye on 40x objective, bring the specimen into focus by adjusting the coarse/fine focusing knob. The machine now will fit the sight of the observer's eyes. (shown in Fig. 7)

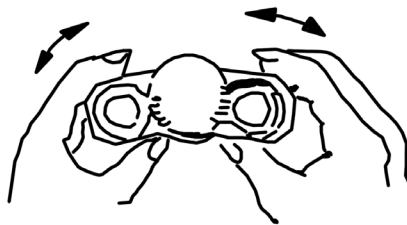


FIG. 6

SIGHT ADJUSTING RING

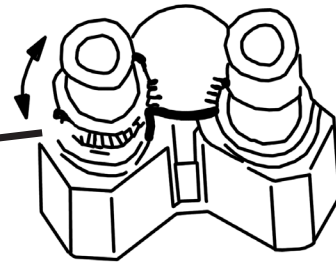


FIG. 7

(3) Coarse/fine focusing

SeilerScope coaxial coarse and fine adjustment knobs make the focusing smoother. To suit operator preference or a heavy or light knob touch, a tension adjustment ring is provided. This device can also prevent the stage slides up. In order to prevent collisions between objective and specimen due to accidental stage movement. The microscope has a focusing limit control knob. Once the specimen is focused, tighten the knob to prevent the stage from moving beyond a safe limit. (shown in Fig. 8)


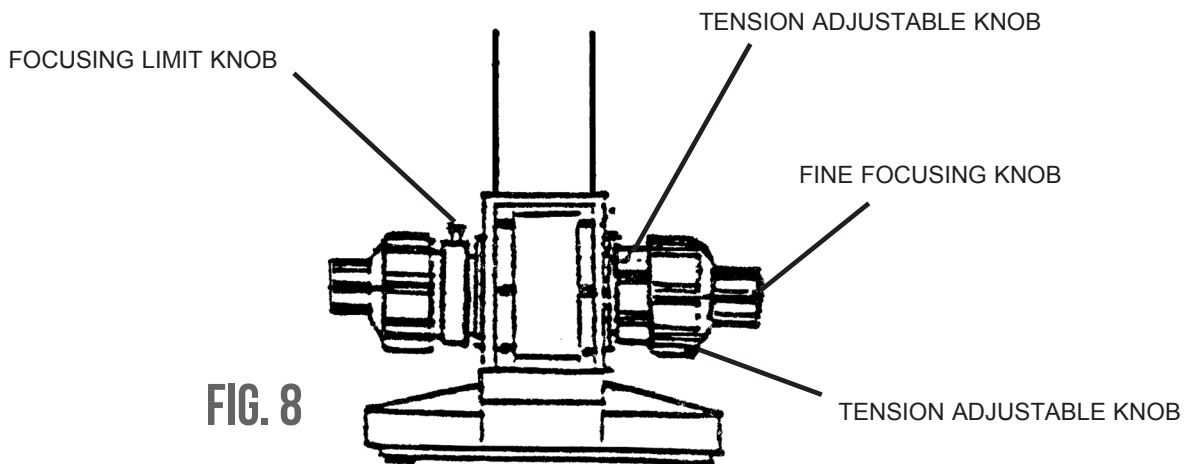


FIG. 8

(4) Stage

The specimen clip which is on the stage hold the specimen very easily. The longitudinal/traverse shifting controller is coaxial and can be used conveniently. (shown in Fig. 9)

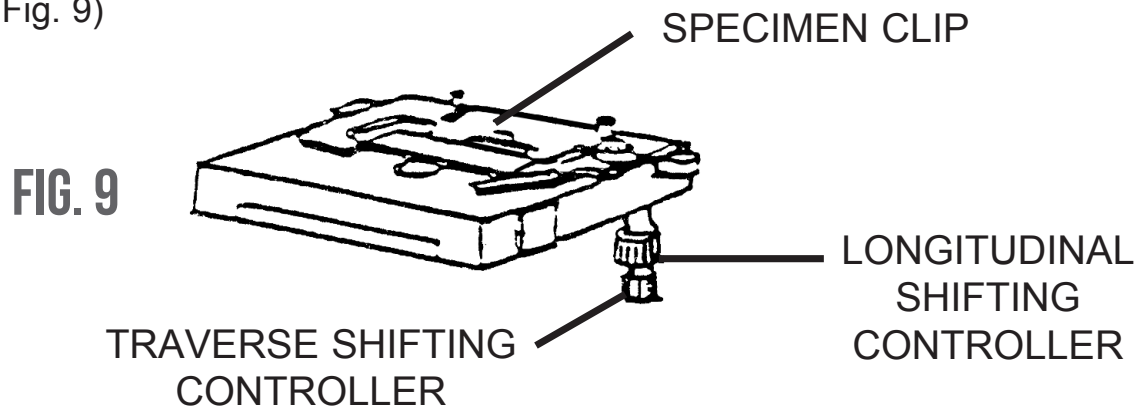

(5) Up/down the condenser

The condenser will move vertically when turning the condenser up/down knob in manner. (shown in Fig. 10)


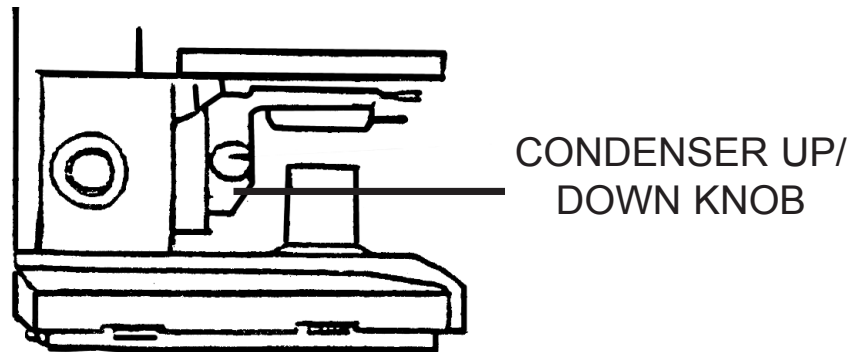


FIG. 10

(6) Utilization of the aperture diaphragm on the condenser.

The numerical aperture of illumination system can be varied by the aperture diaphragm and bring about the change in resolution, contrast and focal depth. Mostly an image of fair contrast may reach, when the diameter of the numerical aperture being 70-80% of the exit pupil of the concerning objective. (shown in Fig. 11)

Removing the eyepieces. Adjust the aperture diaphragm properly while looking through eyepiece tube. The eyepiece tube and the image of the aperture of the bright ring in the objective pupil. Keep in mind the handle position of the aperture diaphragm for each objective when the best image quality is reached.

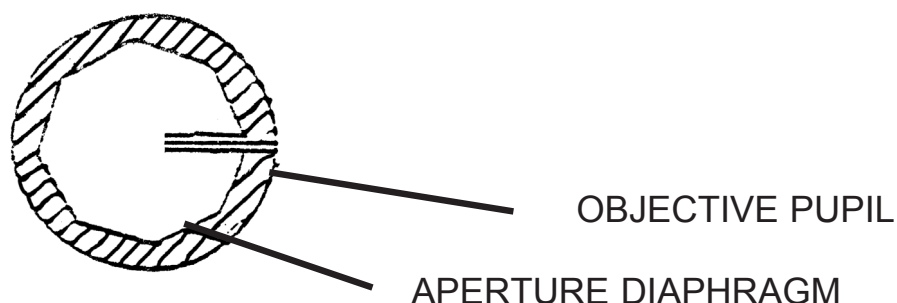

- (7) Power switch and adjusting intensity
Turn on the power, adjusting the intensity knob making the eyes observe image of specimen comfortably.
Note: Don't put the intensity knob on the highest position longly. Avoid deducing life of lamp. (shown in Fig. 12)

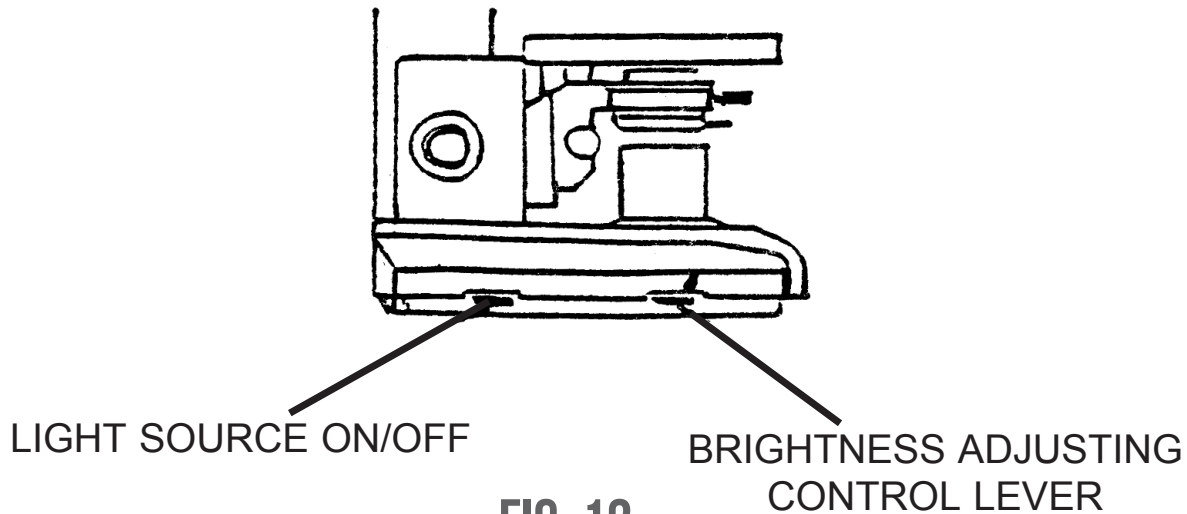


FIG. 12

- (8) Adjusting of field diaphragm
Switch on the power, then turn the 10x objective into the optical axis. Observe with 10x eyepieces. Turning the up/down condenser knob then reach the image of field diaphragm. Then center field diaphragm and optical axis with adjusting screw. Turn the ring of field diaphragm. When the field diaphragm is more than the field of eyepiece. Using 4x objective, then adjust method as so. (shown Fig. 13)

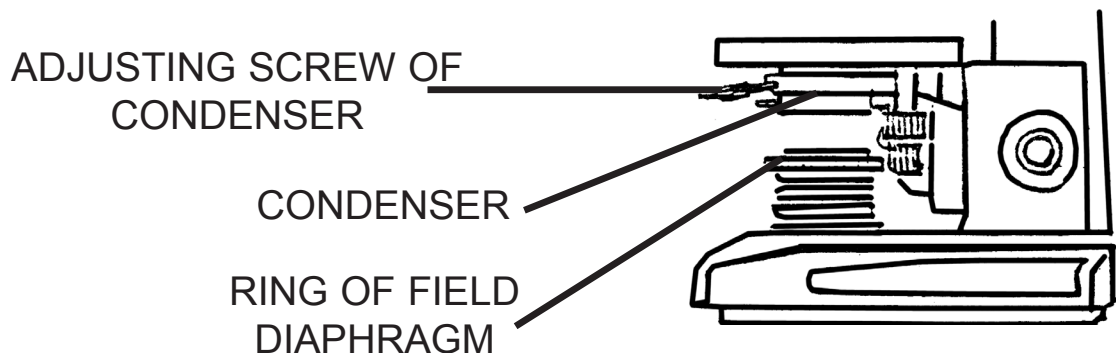


FIG. 13

EXCHANGING THE LAMP AND FUSE

- (1) Pull out the plug of power electrical wire [1] and disconnect the power supply.
- (2) Incline microscope, loosen screw [2] of fixing lamp base board [3] on middle part of bottom, and remove lamp base board from bottom.
- (3) Pull out the old lamp from lamp base [4].
- (4) Insert new lamp [5] into lamp base properly, as shown in Fig. 11 direction, make it touch better.
- (5) Clean the new lamp with absoluted alcohol.
- (6) Refix lamp base board on bottom with screw [2].
- (7) Mount the lamp well. Plug in power source. Turn 4x objective lens into path. Adjust condenser upwards and downwards and make light enter view of field. If light spot is offset the center of view, loose screw [6] slightly and move lamp base [4]. Make lamp spot into center, then tighten up the screw [6] to use immediately. (shown in Fig. 14)

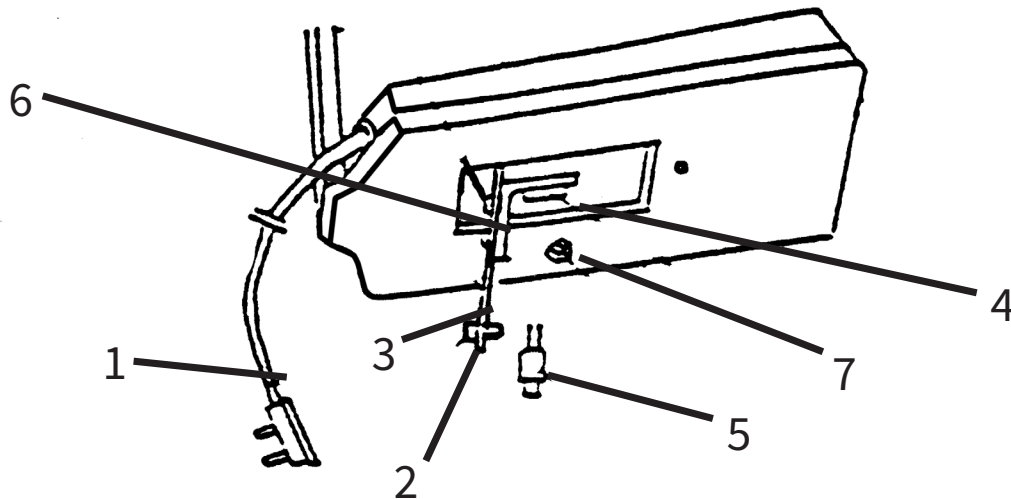


FIG. 14

- (8) Loosen the screw of fuse 7, put out the bad fuse, mount the new fuse. Tighten the screw of fuse and use.

CIRCUIT DIAGRAM

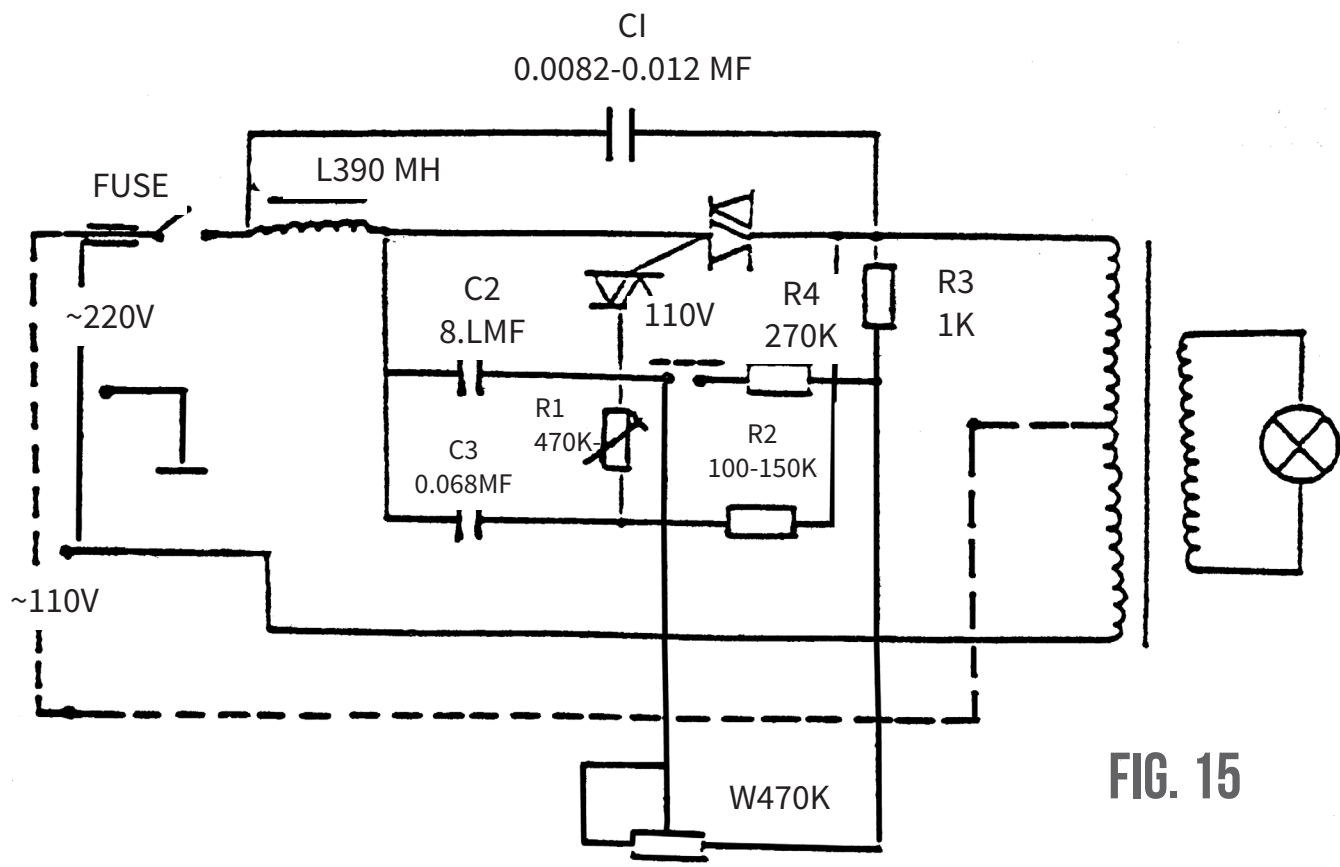


FIG. 15

TIPS & TECHNIQUES

TROUBLESHOOTING THE 40X OBJECTIVE

One of the most common questions the Seiler technicians are asked is what to do when a 40x objective (400x magnification) won't focus or produces a poor image. A poor image on an objective can be caused from a number of problems. By following the simple procedure below, you will be able to troubleshoot about 90% of these problems and get the microscope back in operation:

1. Check the slide. The first step in troubleshooting the 40x objective is make sure the specimen slide is right side up. If the non-cover glass side of the slide is up to the 40x, there will not be enough working distance to focus through the thick glass.
2. Check the cover glass thickness. A cover glass number one (0.17mm thick) is recommended for maximum performance.
3. Make sure the objective is clean. Unscrew the 40x objective and examine it by using a magnifying glass to look at the front lens. To view the front lens, hold the objective in your left hand (if you are right-handed) under good desk lamp or in a well-lit room. Hold the objective vertical with the front lens up (toward the ceiling). Hold the magnifier close to your eye and focus on the very top of the objective. Slowly tilt the tip of the objective toward your eye and away from your eye. At some point you should be able to see dirt or oil on the lens.

To clean the lens, a cleaning solution for 35mm camera lens is recommended. Apply the solution to the dirty or oily lens area with a cotton tipped applicator. Do not rub or scrub the lens. Lightly rotate the applicator between your forefinger and thumb, moving around the lens area. Rotate about three or four times, then discard the dirty applicator. Repeat this at least one more time and then re-examine with the magnifier to check for dirt or oil. If debris is still present, repeat the cleaning procedure.

After cleaning with the solution, breathe warm air onto the lens and use a clean applicator to remove any moisture from the lens. Rotate the applicator lightly on the lens as you did when using the solution. Repeat this two or three times with a clean applicator each time. Re-examine with the magnifier for dirt or oil and repeat the cleaning procedure if debris is still present.

A substitute cleaning solution of mild soap mixed with a large amount of water can be used for temporary cleaning. Make sure the water is not too soapy. Clean cotton gauze can be used in place of cotton tipped applicators using 1" squares, but this generally cleans only the center of the field of view.

4. Call Seiler's Service Department. If the procedures described above do not improve the image of the 40x objective, our Service Department will be happy to provide further assistance.

Dear Purchaser,

Congratulations on the purchase of your microscope. Your instrument has been carefully assembled and shipped to you. Please complete the Warranty Registration online at the link below and answer the questions to activate and guarantee your warranty. Retain this warranty document for your records.

Thank you for purchasing a Seiler microscope.

INTERNATIONAL WARRANTY

Except as set forth in this Three (3) Year International Warranty, Seiler Instrument Company ("SIC") hereby warrants that each Seiler microscope product manufactured and/or sold by SIC shall be free from defects in materials and workmanship under normal use and service for three years. International Warranty includes mechanics, optics, and hardware (such as casters, knobs, tension band). This warranty is non-transferable and is valid only with respect to the original purchaser of the product. SIC obligation under this warranty shall be limited to repairing or replacing, at SIC facility and at SIC expense, any parts or components which are demonstrated to be defective. The purchaser shall be responsible for shipment of the product to SIC facility at 3433 Tree Court Industrial Blvd., St. Louis MO 63122, Attention: Micro Product Department, or such other facility as SIC may otherwise designate. Under certain circumstances which are pre-approved by SIC, necessary repairs may be made at the purchaser's facility. A return authorization is required before returning any product for warranty service by calling 1-800-489-2282 x347.

This warranty shall not apply to electronic and electrical components of the microscope or accessories such as video equipment, monitors and laptop which carry a three (3) year warranty OR any components which are consumable or are required to be replaced or disposed of in normal use of the product, such as lamps, fiber-optic cables and rubber eye cups OR any product which was purchased prior to April 29, 2016.

This warranty shall be void and of no effect: (1) if the product is damaged due to misuse, use in a manner other than pursuant to the instruction for the use of the product, abuse, physical mishandling or natural causes such as flood, fire, earthquake or other perils, as determined by SIC, or (2) if any repairs are made by persons unauthorized by SIC to perform such services.

The warranties set forth here are in lieu of any and all other warranties expressed or implied, including, without limitation, warranties of merchantability and fitness for a particular purpose. Purchaser's rights thereunder are granted in lieu of any other rights purchaser may have and purchaser hereby waives all other rights, warranties, remedies or guarantees whatsoever with respect to the product.

SIC shall not be liable for any reason to any third parties in respect of the product or its performance. Further, SIC shall not be liable for, and purchaser hereby releases SIC from any direct, indirect, consequential, special, incidental or punitive damages in respect to the product. In no event shall SIC be liable for any breach of warranty or other claim in an amount exceeding the purchase price of the product.

The customer is responsible for the shipping costs to Seiler Instrument Company. Seiler Instrument Company will pay the most economical method of shipping back to the customer. Any special shipping method will be paid by the customer.

Warranty must be registered online at:

<http://www.seilermicro.com/products/warranty-registration/>



Toll-Free: 800.489.2282 | Local: 314.968.2282 | Fax: 314.968.3601 | E-mail: micro@seilerinst.com | www.seilerinst.com

Dear Purchaser,

Congratulations on the purchase of your microscope. Your instrument has been carefully assembled and shipped to you. Please complete the Warranty Registration online at the link below and answer the questions to activate and guarantee your warranty. Retain this warranty document for your records.

Thank you for purchasing a Seiler microscope.

LIFETIME WARRANTY

Except as set forth in this Limited Lifetime Warranty, Seiler Instrument Company ("SIC") hereby warrants that each Seiler microscope product manufactured and/or sold by SIC shall be free from defects in materials and workmanship under normal use and service for the life of the product. Lifetime Warranty includes mechanics, optics, hardware (such as casters, knobs, tension band). This warranty is non-transferable and is valid only with respect to the original purchaser of the product. SIC obligation under this warranty shall be limited to repairing or replacing, at SIC facility and at SIC expense, any parts or components which are demonstrated to be defective. The purchaser shall be responsible for shipment of the product to SIC facility at 3433 Tree Court Industrial Blvd., St. Louis MO 63122, Attention: Micro Product Department, or such other facility as SIC may otherwise designate. Under certain circumstances which are pre-approved by SIC, necessary repairs may be made at the purchaser's facility. A return authorization is required before returning any product for warranty service by calling 1-800-489-2282 x347.

This warranty shall not apply to electronic and electrical components of the microscope or accessories such as video equipment, monitors and laptop which carry a three (3) year warranty OR any components which are consumable or are required to be replaced or disposed of in normal use of the product, such as lamps, fiber-optic cables and rubber eye cups OR any product which was purchased prior to April 29, 2016.

This warranty shall be void and of no effect: (1) if the product is damaged due to misuse, use in a manner other than pursuant to the instruction for the use of the product, abuse, physical mishandling or natural causes such as flood, fire, earthquake or other perils, as determined by SIC, or (2) if any repairs are made by persons unauthorized by SIC to perform such services.

The warranties set forth here are in lieu of any and all other warranties expressed or implied, including, without limitation, warranties of merchantability and fitness for a particular purpose. Purchaser's rights thereunder are granted in lieu of any other rights purchaser may have and purchaser hereby waives all other rights, warranties, remedies or guarantees whatsoever with respect to the product.

SIC shall not be liable for any reason to any third parties in respect of the product or its performance. Further, SIC shall not be liable for, and purchaser hereby releases SIC from any direct, indirect, consequential, special, incidental or punitive damages in respect to the product. In no event shall SIC be liable for any breach of warranty or other claim in an amount exceeding the purchase price of the product.

The customer is responsible for the shipping costs to Seiler Instrument Company. Seiler Instrument Company will pay the most economical method of shipping back to the customer. Any special shipping method will be paid by the customer.

Warranty must be registered online at:

<http://www.seilermicro.com/products/warranty-registration/>



Toll-Free: 800.489.2282 | Local: 314.968.2282 | Fax: 314.968.3601 | E-mail: micro@seilerinst.com | www.seilerinst.com



3433 Tree Court Industrial Blvd.
St. Louis, MO 63122
USA

Toll-Free: 800-489-2282
Local: 314-968-2282
Fax: 314-968-3601
Email: micro@seilerinst.com
Web: www.seilermicro.com